



# DEBITBAC

Acc. To ISO 1438/1 - 1980.

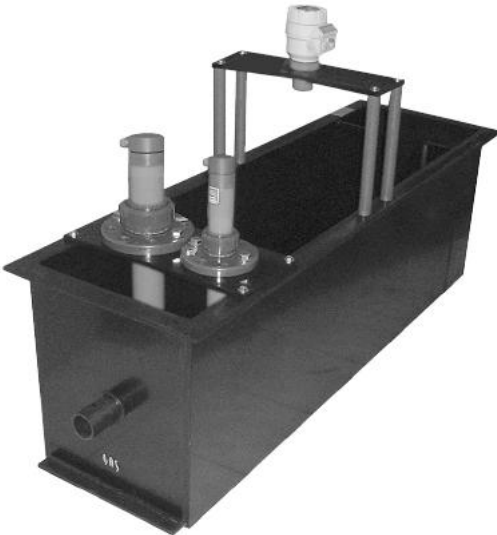

## RECOMMENDATIONS

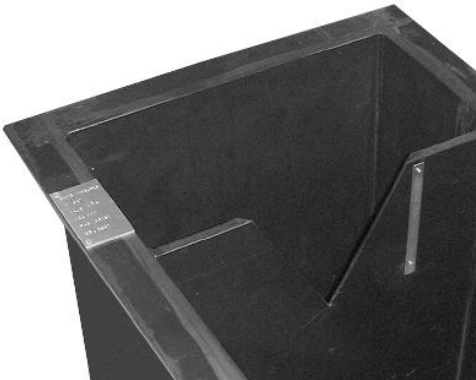

**BAMO MESURES**

22, Rue de la Voie des Bans - 95 100 ARGENTEUIL - FRANCE  
Tel.: +33 1 30 25 83 20 - E-mail: [info@bamo.fr](mailto:info@bamo.fr)  
Fax: +33 1 34 10 16 05 - <http://www.bamo.eu>

**DEBITBAC**  
16-05-2007 755 M

**MSA**  
755-02/1

## INSTALLATION

- All parts of the DEBITBAC and all accessories should be easy to access for inspection and maintenance.
- The plates as for thin type should have a chamfered edge (45° angle) downstream side.
- The plate thick depends of its width and of height of fluid (due to the flow). Commonly the thick is 6, 8 or 12 mm.
- A limnometric scale must be visible easily at any time for evaluation of water level.
- All instrumentation should be installed in the tranquilization basin or in a measuring well.
- The dimensions of the complete device should correspond to 70%...10% of maximal capacity.  
Over dimensions may induce a bad accuracy for low flow rates.

## MAINTENANCE

The plate must be keep cleaned without fouling, micro-organisms etc. and during winter time free of ice.

If necessary, precautions to prevent sedimentation or accumulation of sludge may be organized.

The zero level for the transmitter has to be checked regularly with a null flow rate. If this flow condition is not possible, a specific graduated ruler for standardization must be installed.

Other check points:

- Plate aspect, integrity
- Plate crest horizontality
- Plate verticality
- crest height vs. a well known level point (to detect a possible sinking of the complete system).

## TECHNICAL FEATURES

- Flow rate from 1 m<sup>3</sup>/h up to 400 m<sup>3</sup>/h
- V from 20° to 100°
- Realization to specific dimensions
- Ready to use
- According to ISO 1438/1-1980
- Construction: PVC and/or PEHD

## DIMENSIONS

In respect to Kindvater-shen formula some physical limits exist (ISO 1438/1-1980).

LP = 4 to 5 time h max.

LT = 10 time b


HT = p + h max. + 0.05 m

h > 0.06 m

p > 0.09 m

Other limits:

See the data sheet of your DEBITBAC.

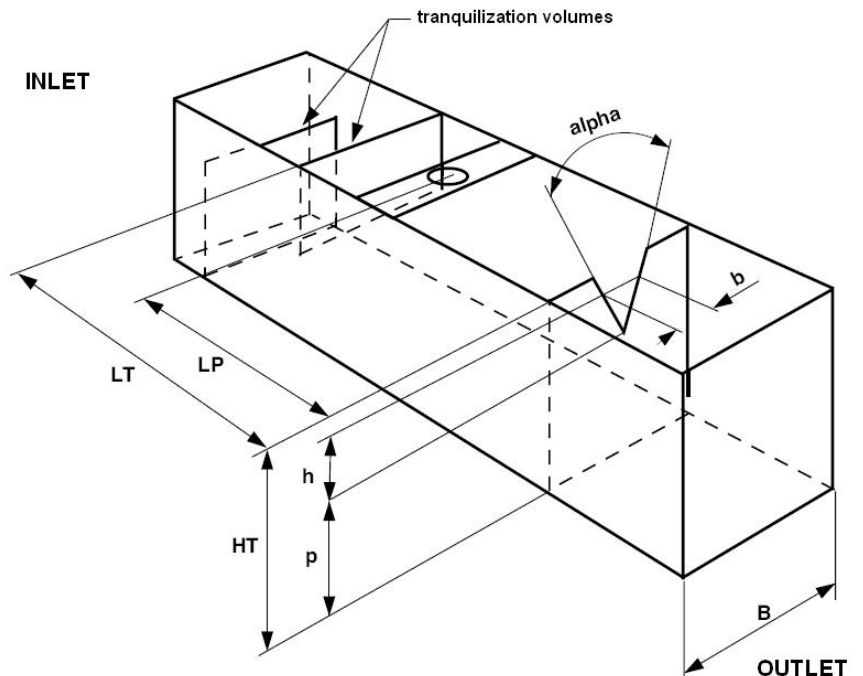

# BAMO MESURES

22, Rue de la Voie des Bans - 95 100 ARGENTEUIL - FRANCE

Tel.: +33 1 30 25 83 20 - E-mail: info@bamo.fr

Fax: +33 1 34 10 16 05 - http://www.bamo.eu

DEBITBAC

16-05-2007

755 M

MSA

755-02/1